




Private and Confidential

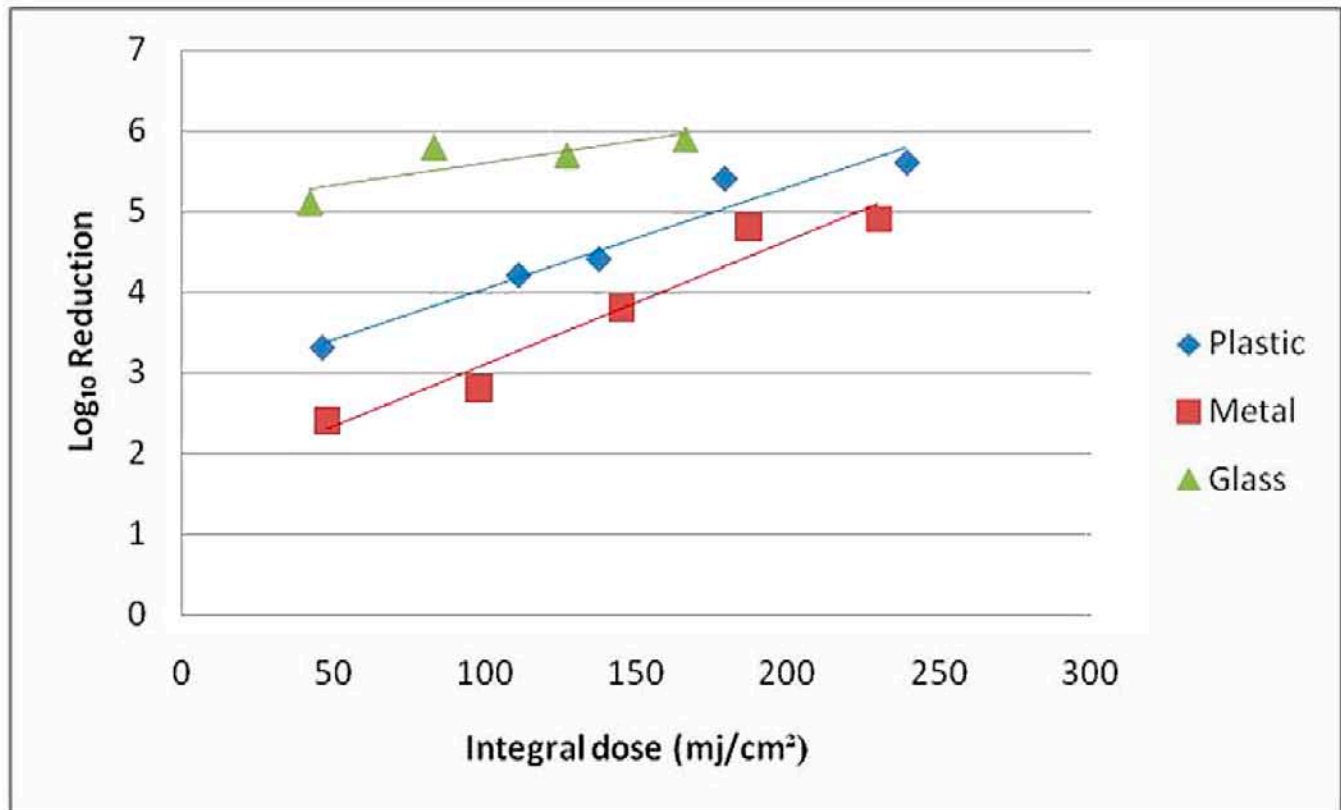

Log reduction of *A. baumannii* NCTC 12156 on plastic, metal and glass after exposure to Far UV with the **smooth** setting

NOTE BY HEI:

THE METAL USED FOR THIS TEST WAS ROUGH STEEL COUPONS. HEI FEELS THAT RESULTS WOULD HAVE BEEN CLOSER TO GLASS IF THESE TESTS WERE PERFORMED ON STAINLESS STEEL THAT IS FOUND IN MOST HEALTH CARE FACILITIES.